



FIRMS - Forensic Isotope Ratio Mass Spectrometry PT Scheme

Round: 245

Issue Number 1

Issued 10 November 2016



Science
for a safer world

LGC | 1 Chamberhall Business Park | Chamberhall Green | Bury | Lancashire | BL9 0AP | UK |
+44(0)161 762 2500 | ptcustomerservices@LGCGroup.com | www.lgcstandards.com

LGC is the accredited provider of the PT scheme.



0001

Scheme Information

Aims of Scheme

The primary aim of the Forensic Isotope Ratio Mass Spectrometry Proficiency Testing Scheme (FIRMS) is to enable laboratories performing isotope ratio analysis of a range of test materials to monitor their performance and compare it with that of their peers. The FIRMS scheme also aims to provide information to participants on technical issues and methodologies relating to isotope ratio analysis.

Further information on the scheme organisation, the test materials, and the statistical analysis of data are available in the FIRMS Scheme Description and the LGC PT General Protocol.

Performance Assessment

Once a PT round has closed, the results will be analysed and the assigned value determined for each analyte, according to the criteria provided in the Scheme Description. Information regarding the traceability of each calculated assigned value is also provided in the Scheme Description.

For quantitative data, the participant's result, x , (or $\log_{10} x$ for microbiological data) is converted into a z score using the following formula;

$$z = \frac{(x - X)}{\text{SDPA}}$$

X = Assigned value
SDPA = Standard deviation for proficiency assessment

For quantitative data, the uncertainty of the assigned value is calculated to ensure that it would have a negligible effect on participants' performance scores. If the uncertainty of the assigned value is greater than $0.3 \times \text{SDPA}$, then this is not considered negligible. In this situation, a z' (z prime) performance score is automatically calculated rather than a z score, in order to take account of the measurement uncertainty of the assigned value. The z' score is calculated using the following formula;

$$z' = \frac{(x - X)}{\sqrt{(\text{SDPA}^2 + UxAV^2)}}$$

X = Assigned value
SDPA = Standard deviation for proficiency assessment
 $UxAV$ = Uncertainty of the assigned value

$$\text{Expanded SDPA} = \sqrt{(\text{SDPA}^2 + UxAV^2)}$$

Trend graphs will use a mixture of z and z' scores, i.e. the 'performance score' for the round.

For quantitative data, gross errors or blunders are removed from the data by removal of any results that are greater than the assigned value $\pm 5 \times \text{SDPA}$. These results are not used in the final calculation of the assigned value and other summary statistics and will be included in the number of 'Excluded Results'. All results, including excluded results, will be given a performance score.

For the purposes of performance assessment for a single round, z and z' scores are interpreted as follows:

| z/z' score | Interpretation | Colour coding |
|---------------------------|-----------------------|------------------|
| $ z \leq 2.00$ | Satisfactory result | Green |
| $2.00 < z $ and < 3.00 | Questionable result | Amber |
| $ z \geq 3.00$ | Unsatisfactory result | Red |
| No score given | See below | No colour coding |

Performance scores will not be given for the following:

- For qualitative results, where satisfactory performance is based on the participants reporting the same result as the assigned result. E.g. detected, not detected. For these results, colour coding of green (satisfactory) or red (unsatisfactory) will apply.
- For results of zero; such a result is not normally appropriate and should not be reported, the result should be reported as less than the detection limit rather than zero.
Note: for a very small number of analytes it may be appropriate to report a result of zero, depending on the type of measurement scale being used.
- For quantitative results where the analyte under test is present in the test material but participants report zero results or greater than results. In these cases, it is not possible to allocate a performance score and participants should assess their performance based on the assigned value and satisfactory range given.
- For quantitative results where the analyte under test is present in the test material but participants report a 'less than' value. In these cases, it is not possible to allocate a numeric performance score, however, where the 'less than' value reported is $< (AV - 3 \times \text{SDPA})$ the 'less than' value will be assessed as unsatisfactory (red colour coding), where the less than value reported is between $< (AV - 3 \times \text{SDPA})$ and $< (AV - 2 \times \text{SDPA})$, or $> (AV + 2 \times \text{SDPA})$ the assessment will be questionable (orange colour coding) and it is recommend that you assess whether the method used is fit for purpose, and where the less than value reported is between $(AV - 2 \times \text{SDPA})$ and $(AV + 2 \times \text{SDPA})$ a satisfactory assessment (green colour coding) will be given as such results are deemed to be consistent with the assigned value.
- For quantitative results, for microbiological test materials, where the analyte under test is not present in the test material, the assigned value will be classified as 'Absent'. Results reported as 'less than' at or below the detection level for our method of confirmation will be assessed as satisfactory (green colour code). Results reported at a higher detection level will not be assessed and participants will need to use their own judgement to determine whether their result is fit for its intended use. Results reporting a positive count will be assessed as unsatisfactory (red colour code).
- For quantitative results, for chemistry or clinical test materials, where the analyte under test has not been spiked into the test material, the assigned value will be classified as 'Zero Spike'. A 'less than' value reported at or below the detection level, set as the assigned

value, will be assessed as satisfactory (green colour code). A 'less than' value reported above the detection level will not be assessed and participants will need to use their own judgement to determine whether their result is fit for its intended use. Positive, numeric, results which are below the detection level, set as the assigned value, will not be assessed, whilst those that are greater than the assigned value will be assessed as unsatisfactory (red colour code).

In some cases, performance scores may not be provided or may be provided but with colour coding suspended (indicating that scores need to be interpreted with caution). For example:

- For small data sets where less than 8 results have been submitted and the assigned value is derived using a consensus value from the participants' results. In these circumstances, there may be increased uncertainty of the assigned value, given the low number of participants, and performance scores will be given for information only.
- In cases where the distribution of the results gives cause for concern e.g. bi-modal data sets. These circumstances will be dependent on the statistical design that is in place.
- If the assigned value falls below a concentration threshold (only applies to some schemes).

In these or similar circumstances, further explanation as to the reasons for suspension of performance scoring or colour coding, and on the interpretation of results, will be given in the report.

Note: Data displayed in the report will have been rounded to the required number of decimal places. However statistical calculations will have been performed on unrounded data. For this reason, there may appear to be differences between displayed data and calculated data, but this does not affect results in any way.

Confidentiality

A unique laboratory reference code is used to report results in order to ensure confidentiality

Contact details

The Technical Scheme Coordinator is Wayne Gaunt

Please contact ptcustomerservices@gcggroup.com if you have any questions or comments regarding the scheme.

Authorisation

This report was authorised by Matthew Whetton, Head of Chemistry on the 10 November 2016



Sample Details

Samples were despatched on 26 September 2016
The reporting deadline was 04 November 2016.

The following samples were distributed in FIRMS Round 245:

- 1: 1 x 0.5g caffeine for the determination of delta 2H, 13C, 15N and 18O
2: 1 x 0.5g propylene glycol for the determination of delta 2H, 13C and 18O

Further information regarding assigned values, performance assessment and technical comments can be found under the individual sample and analyte results.

Calculated within and between participant standard deviations

Sample 1 (caffeine)

| Analyte | Within participant SD | Between participant SD |
|-----------|-----------------------|------------------------|
| Delta 2H | 10.4325 | 1.7815 |
| Delta 13C | 0.0521 | 0.0773 |
| Delta 15N | 0.0679 | 0.0565 |
| Delta 18O | 0.3984 | 0.0451 |

Sample 2 (propylene glycol)

| Analyte | Within participant SD | Between participant SD |
|-----------|-----------------------|------------------------|
| Delta 2H | 2.2580 | 1.9027 |
| Delta 13C | 0.0972 | - |
| Delta 18O | 0.9361 | 0.3956 |

Quality Control

All homogeneity assessments have been conducted in accordance with the principles stipulated in ISO 13528 [1]. Further details regarding the assessment of homogeneity can be found in the LGC Standards Proficiency Testing General Protocol.

| Sample | Analyte/Test | Result (SD) | Assessment |
|----------------------|--------------|----------------|------------|
| 1 (caffeine) | delta 13C | -39.42 (0.044) | Pass |
| 2 (propylene glycol) | delta 13C | -27.17 (0.063) | Pass |

*Results were scaled to the NBS19-LSVEC scale.

Analysis carried out for the purposes of homogeneity and stability testing were sub-contracted by LGC to an external laboratory.

For quantitative testing in this round, a comparison of the standard deviation of the homogeneity results returned and the SDPA expected for the participant assessment was carried out. The samples were considered to be sufficiently homogeneous for use in the PT scheme, based on the values returned.

For qualitative testing, the target analyte must be detected in 100% of test materials analysed.

For any analyte which has not been proven to be sufficiently homogeneous, and any closely related analytes, the value set for the SDPA may be suspended in order to take account of any potential inhomogeneity. The actual value used for the standard deviation for proficiency assessment is shown at the foot of the results and z-score tables in this report.

Often a particular test material does not require homogeneity assessment prior to distribution. Such sample types include standard solutions and aqueous solutions.

[1] ISO 13528 (2015), 'Statistical methods for use in proficiency testing by inter-laboratory comparisons'.

Sample: 01 - FIRMS sample 1**Analyte: delta 2H (VSMOW)**

| Lab ID | Method | Result | z score |
|--------|---------------------------------|---------|---------|
| FM0002 | Isotope Ratio Mass Spectrometry | -117.20 | |
| FM0010 | Isotope Ratio Mass Spectrometry | -138.21 | |
| FM0014 | Isotope Ratio Mass Spectrometry | -117.06 | |
| FM0016 | Isotope Ratio Mass Spectrometry | -129.47 | |
| FM0018 | Isotope Ratio Mass Spectrometry | -121.42 | |
| FM0028 | Isotope Ratio Mass Spectrometry | -147.90 | |
| FM0041 | Isotope Ratio Mass Spectrometry | -122.73 | |

Data Statistics

| | Value |
|----------------------------|--------------------|
| Number of Results | 7 |
| Number of Excluded Results | 0 |
| Mean | N/A |
| Median | N/A |
| Standard Deviation | N/A |
| Robust Standard Deviation | N/A |
| Result Range | -147.90 to -117.06 |

Comments

The participants in the FIRMS scheme were allowed to report up to 10 results, for the purposes of calculating individual and group summary statistics, plus a mean result, which was used to calculate the summary statistics subsequently applied in the assessment of performance.

Generally the data reported was good for most analytes; however a wide range of values from -117.06 to -147.90 were reported for delta 2H for sample 1. As there is little comparability an assigned value cannot be provided and so performance scores have been removed and the results have been included in the report for information purposes only.

The SDPA values used in the determination of performance scores for both delta 13C and delta 15N are set at fixed values of 0.15; whereas the SDPA values for delta 2H and delta 18O are derived using the robust standard deviation of the data returned. Generally the robust standard deviation is larger for both delta 2H and delta 18O and so a wider range of results will therefore be assessed as satisfactory for these analytes.

Participants are advised to consider the magnitude of the SDPA values used, and the absolute difference of their result from the assigned value, when interpreting their performance.

Sample: 01 - FIRMS sample 1

Analyte: delta 13C (VPDB)


| Lab ID | Method | Result | z score |
|--------|---------------------------------|--------|---------|
| FM0002 | Isotope Ratio Mass Spectrometry | -39.26 | -0.20 |
| FM0003 | Isotope Ratio Mass Spectrometry | -39.33 | -0.67 |
| FM0010 | Isotope Ratio Mass Spectrometry | -39.25 | -0.13 |
| FM0011 | Isotope Ratio Mass Spectrometry | -39.33 | -0.67 |
| FM0014 | Isotope Ratio Mass Spectrometry | -39.21 | 0.13 |
| FM0016 | Isotope Ratio Mass Spectrometry | -39.64 | -2.73 |
| FM0018 | Isotope Ratio Mass Spectrometry | -39.20 | 0.20 |
| FM0028 | Isotope Ratio Mass Spectrometry | -39.18 | 0.33 |
| FM0033 | Isotope Ratio Mass Spectrometry | -39.17 | 0.40 |
| FM0035 | Isotope Ratio Mass Spectrometry | -39.23 | 0.00 |
| FM0037 | Isotope Ratio Mass Spectrometry | -39.15 | 0.53 |
| FM0041 | Isotope Ratio Mass Spectrometry | -38.37 | 5.73 |

Data Statistics

| | Value |
|----------------------------|------------------|
| Number of Results | 12 |
| Number of Excluded Results | 1 |
| Mean | -39.27 |
| Median | -39.23 |
| Standard Deviation | 0.137 |
| Robust Standard Deviation | 0.074 |
| Result Range | -39.64 to -39.15 |

Performance Statistics

| | Value |
|-------------------------------|------------------|
| Assigned Value | -39.23 |
| Uncertainty of Assigned Value | 0.03 |
| SDPA | 0.15 |
| Satisfactory Range | -39.53 to -38.93 |
| Satisfactory z scores | 83.3% |
| Questionable z scores | 8.3% |
| Unsatisfactory z scores | 8.3% |

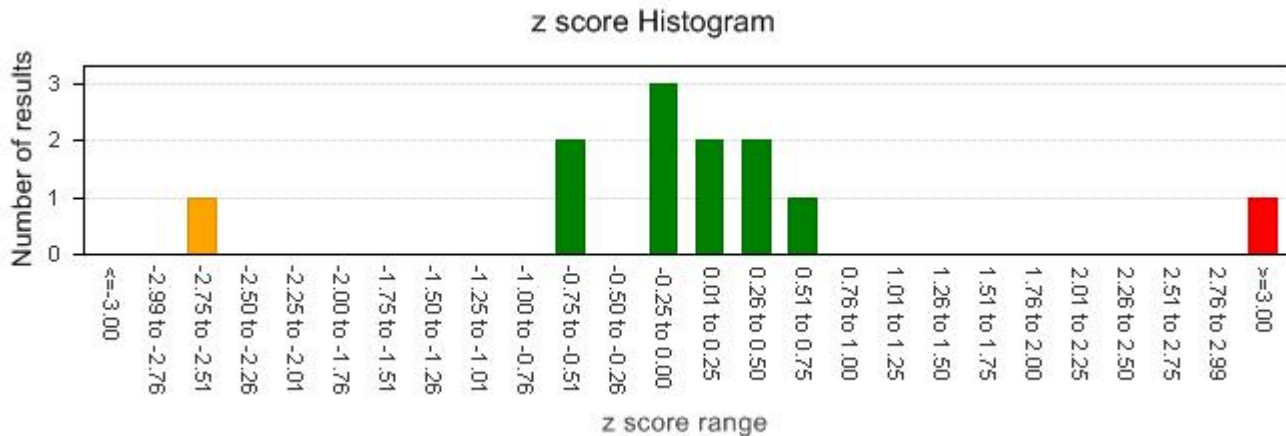

Methodology Summary

| Method | Number of Results | Excluded Results | % of Total | Median | Robust SD | Range | Sat. |
|---------------------------------|-------------------|------------------|------------|--------|-----------|------------------|------|
| | | | | | | | % |
| Isotope Ratio Mass Spectrometry | 12 | 1 | 100 | -39.23 | 0.074 | -39.64 to -39.15 | 83.3 |
| All | 12 | 1 | 100 | -39.23 | 0.074 | -39.64 to -39.15 | 83.3 |

Comments

Sample: 01 - FIRMS sample 1

Analyte: delta 15N (AIR)


| Lab ID | Method | Result | z' score* |
|--------|---------------------------------|--------|-----------|
| FM0002 | Isotope Ratio Mass Spectrometry | -9.77 | 1.82 |
| FM0011 | Isotope Ratio Mass Spectrometry | -10.16 | -0.21 |
| FM0014 | Isotope Ratio Mass Spectrometry | -10.12 | 0.00 |
| FM0016 | Isotope Ratio Mass Spectrometry | -10.12 | 0.00 |
| FM0018 | Isotope Ratio Mass Spectrometry | -10.37 | -1.30 |
| FM0028 | Isotope Ratio Mass Spectrometry | -10.25 | -0.68 |
| FM0033 | Isotope Ratio Mass Spectrometry | -9.80 | 1.67 |
| FM0035 | Isotope Ratio Mass Spectrometry | -9.77 | 1.82 |

Data Statistics

| | Value |
|----------------------------|-----------------|
| Number of Results | 8 |
| Number of Excluded Results | 0 |
| Mean | -10.05 |
| Median | -10.12 |
| Standard Deviation | 0.234 |
| Robust Standard Deviation | 0.282 |
| Result Range | -10.37 to -9.77 |

Performance Statistics

| | Value |
|-------------------------------|-----------------|
| Assigned Value | -10.12 |
| Uncertainty of Assigned Value | 0.12 |
| SDPA | 0.15 |
| Expanded SDPA | 0.192 |
| Satisfactory Range | -10.50 to -9.74 |
| Satisfactory z' scores | 100.0% |
| Questionable z' scores | 0.0% |
| Unsatisfactory z' scores | 0.0% |

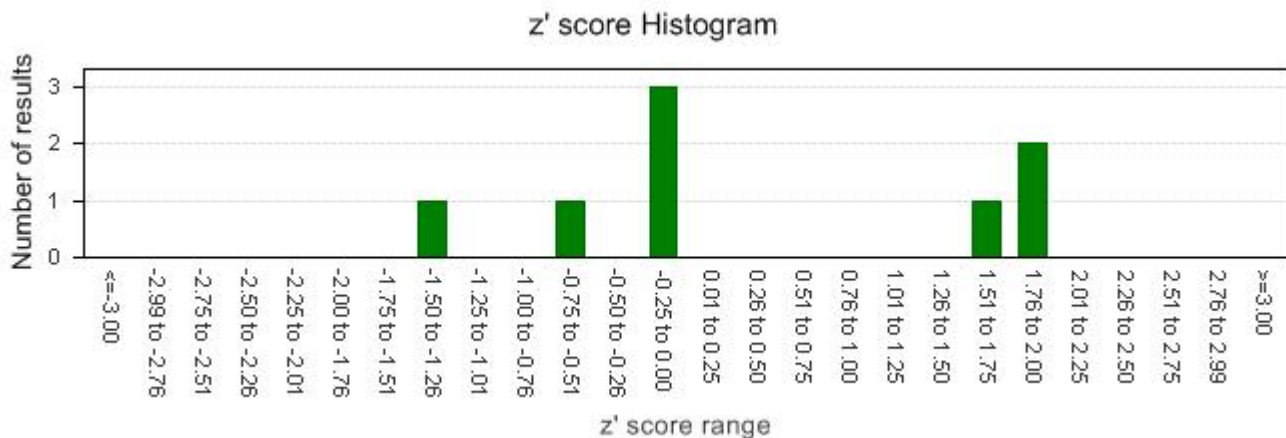

Methodology Summary

| Method | Number of Results | Excluded Results | % of Total | Median | Robust SD | Range | Sat. |
|---------------------------------|-------------------|------------------|------------|--------|-----------|-----------------|-------|
| | | | | | | | % |
| Isotope Ratio Mass Spectrometry | 8 | 0 | 100 | -10.12 | 0.282 | -10.37 to -9.77 | 100.0 |
| All | 8 | 0 | 100 | -10.12 | 0.282 | -10.37 to -9.77 | 100.0 |

Comments

*Please note, participant performance for this analyte has been assessed using a z' score, rather than a z score, in order to account for the measurement uncertainty of the assigned value which is not negligible when compared to the SDPA.

Sample: 01 - FIRMS sample 1**Analyte: delta 18O (VSMOW)**

| Lab ID | Method | Result | z' score* |
|--------|---------------------------------|--------|-----------|
| FM0002 | Isotope Ratio Mass Spectrometry | 20.55 | 0.04 |
| FM0011 | Isotope Ratio Mass Spectrometry | 21.52 | 0.71 |
| FM0016 | Isotope Ratio Mass Spectrometry | 19.13 | -0.93 |
| FM0018 | Isotope Ratio Mass Spectrometry | 21.21 | 0.49 |
| FM0033 | Isotope Ratio Mass Spectrometry | 17.97 | -1.73 |
| FM0035 | Isotope Ratio Mass Spectrometry | 20.43 | -0.04 |

Due to the low number of results returned, performance scores are shown for information purposes only

Data Statistics

| | Value |
|----------------------------|----------------|
| Number of Results | 6 |
| Number of Excluded Results | 0 |
| Mean | 20.14 |
| Median | 20.49 |
| Standard Deviation | 1.344 |
| Robust Standard Deviation | 1.298 |
| Result Range | 17.97 to 21.52 |

Performance Statistics

| | Value |
|-------------------------------|----------------|
| Assigned Value | 20.49 |
| Uncertainty of Assigned Value | 0.66 |
| SDPA | 1.298 |
| Expanded SDPA | 1.456 |
| Satisfactory Range | 17.58 to 23.40 |
| Satisfactory z' scores | 100.0% |
| Questionable z' scores | 0.0% |
| Unsatisfactory z' scores | 0.0% |

Methodology Summary

| Method | Number of Results | Excluded Results | % of Total | Median | Robust SD | Range | Sat. |
|---------------------------------|-------------------|------------------|------------|--------|-----------|----------------|-------|
| | | | | | | | % |
| Isotope Ratio Mass Spectrometry | 6 | 0 | 100 | 20.49 | 1.298 | 17.97 to 21.52 | 100.0 |
| All | 6 | 0 | 100 | 20.49 | 1.298 | 17.97 to 21.52 | 100.0 |

Comments

*Please note, participant performance for this analyte has been assessed using a z' score, rather than a z score, in order to account for the measurement uncertainty of the assigned value which is not negligible when compared to the SDPA.

Sample: 02 - FIRMS sample 2**Analyte: delta 2H (VSMOW)**

| Lab ID | Method | Result | z score |
|--------|---------------------------------|--------|---------|
| FM0002 | Isotope Ratio Mass Spectrometry | -46.15 | |
| FM0016 | Isotope Ratio Mass Spectrometry | -50.24 | |
| FM0018 | Isotope Ratio Mass Spectrometry | -48.98 | |
| FM0028 | Isotope Ratio Mass Spectrometry | -48.70 | |
| FM0035 | Isotope Ratio Mass Spectrometry | -46.85 | |
| FM0041 | Isotope Ratio Mass Spectrometry | -65.01 | |

Data Statistics

| | Value |
|----------------------------|------------------|
| Number of Results | 6 |
| Number of Excluded Results | 0 |
| Mean | N/A |
| Median | N/A |
| Standard Deviation | N/A |
| Robust Standard Deviation | N/A |
| Result Range | -65.01 to -46.15 |

Comments

Please refer to caffeine, delta 2H for the general report comments.

Generally the data reported was good for most analytes in sample 2; however there was little comparability for delta 2H (VSMOW) and so an assigned value could not be provided. Therefore performance scores have been removed and the results have been included in the report for information purposes only.

Sample: 02 - FIRMS sample 2

Analyte: delta 13C (VPDB)


| Lab ID | Method | Result | z score |
|--------|---------------------------------|--------|---------|
| FM0002 | Isotope Ratio Mass Spectrometry | -27.32 | -0.47 |
| FM0003 | Isotope Ratio Mass Spectrometry | -27.24 | 0.07 |
| FM0014 | Isotope Ratio Mass Spectrometry | -27.32 | -0.47 |
| FM0016 | Isotope Ratio Mass Spectrometry | -27.51 | -1.73 |
| FM0018 | Isotope Ratio Mass Spectrometry | -27.23 | 0.13 |
| FM0028 | Isotope Ratio Mass Spectrometry | -27.25 | 0.00 |
| FM0033 | Isotope Ratio Mass Spectrometry | -27.06 | 1.27 |
| FM0035 | Isotope Ratio Mass Spectrometry | -27.34 | -0.60 |
| FM0037 | Isotope Ratio Mass Spectrometry | -27.13 | 0.80 |
| FM0041 | Isotope Ratio Mass Spectrometry | -27.24 | 0.07 |

Data Statistics

| | Value |
|----------------------------|------------------|
| Number of Results | 10 |
| Number of Excluded Results | 0 |
| Mean | -27.26 |
| Median | -27.25 |
| Standard Deviation | 0.122 |
| Robust Standard Deviation | 0.111 |
| Result Range | -27.51 to -27.06 |

Performance Statistics

| | Value |
|-------------------------------|------------------|
| Assigned Value | -27.25 |
| Uncertainty of Assigned Value | 0.04 |
| SDPA | 0.15 |
| Satisfactory Range | -27.55 to -26.95 |
| Satisfactory z scores | 100.0% |
| Questionable z scores | 0.0% |
| Unsatisfactory z scores | 0.0% |

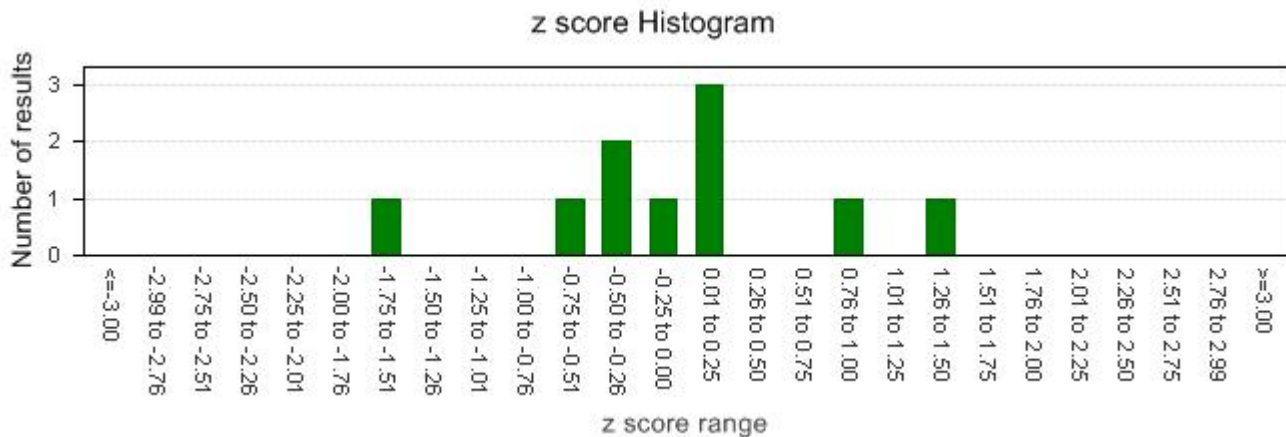

Methodology Summary

| Method | Number of Results | Excluded Results | % of Total | Median | Robust SD | Range | Sat. |
|---------------------------------|-------------------|------------------|------------|--------|-----------|------------------|-------|
| | | | | | | | % |
| Isotope Ratio Mass Spectrometry | 10 | 0 | 100 | -27.25 | 0.111 | -27.51 to -27.06 | 100.0 |
| All | 10 | 0 | 100 | -27.25 | 0.111 | -27.51 to -27.06 | 100.0 |

Comments

Sample: 02 - FIRMS sample 2**Analyte: delta 18O (VSMOW)**

| Lab ID | Method | Result | z' score* |
|--------|---------------------------------|--------|-----------|
| FM0002 | Isotope Ratio Mass Spectrometry | -13.29 | -0.18 |
| FM0016 | Isotope Ratio Mass Spectrometry | -13.94 | -0.96 |
| FM0018 | Isotope Ratio Mass Spectrometry | -10.31 | 3.41 |
| FM0035 | Isotope Ratio Mass Spectrometry | -12.99 | 0.18 |

Due to the low number of results returned, performance scores are shown for information purposes only

Data Statistics

| | Value |
|----------------------------|------------------|
| Number of Results | 4 |
| Number of Excluded Results | 0 |
| Mean | -12.63 |
| Median | -13.14 |
| Standard Deviation | 1.598 |
| Robust Standard Deviation | 0.704 |
| Result Range | -13.94 to -10.31 |

Performance Statistics

| | Value |
|-------------------------------|------------------|
| Assigned Value | -13.14 |
| Uncertainty of Assigned Value | 0.44 |
| SDPA | 0.704 |
| Expanded SDPA | 0.830 |
| Satisfactory Range | -14.80 to -11.48 |
| Satisfactory z' scores | 75.0% |
| Questionable z' scores | 0.0% |
| Unsatisfactory z' scores | 25.0% |

Methodology Summary

| Method | Number of Results | Excluded Results | % of Total | Median | Robust SD | Range | Sat. |
|---------------------------------|-------------------|------------------|------------|--------|-----------|------------------|------|
| | | | | | | | % |
| Isotope Ratio Mass Spectrometry | 4 | 0 | 100 | -13.14 | 0.704 | -13.94 to -10.31 | 75.0 |
| All | 4 | 0 | 100 | -13.14 | 0.704 | -13.94 to -10.31 | 75.0 |

Comments

*Please note, participant performance for this analyte has been assessed using a z' score, rather than a z score, in order to account for the measurement uncertainty of the assigned value which is not negligible when compared to the SDPA.